

**CP SERIES INDUSTRIAL USE pH•ORP•ION ELECTRODES**

CP series industrial use pH/ORP/ion electrodes are KCl non-supply type electrodes. These electrodes are the result of continuous research and development and offer high performance, ease of installation and low maintenance requirements. The electrodes are compatible with DKK-TOA's transmitters that have a temperature compensation function based on a 10kΩ (at 25°C) sensor. These electrodes can be incorporated into immersion type holders, flow through type holders or dip-in type guide pipes. The process connection is a universal pipe thread (Rc<sup>3</sup>/<sub>4</sub>), allowing compatible holders and guide pipes to be easily obtained by users.

The inner liquid non-supply type electrodes eliminate the need to refill with KCl solution and also the need for pressure compensation. The reference electrode has a newly developed gel-type inner liquid and a specially designed porous PTFE liquid junction. These features offer a wider operating temperature, increased electrode life and liquid junction potential characteristics and also eliminate the problem of electrodes drying up during storage.

The measuring electrode uses an easily replaceable sensor chip. Even under harsh operating conditions, it will not be required to replace the whole electrode. Only the sensor chip requires replacement, thus reducing running costs and providing excellent cost of ownership advantages. Replacement of the sensor chip is straightforward and it is even possible to change the sensor chip with a different type after field installation.



**COMPATIBLE TRANSMITTERS**

CP series industrial use pH/ORP/F-ion electrodes can be used in combination with the following transmitters which have a temperature compensation function based on a 10kΩ (at 25°C) temperature sensor.

Type of electrode	Compatible transmitters
pH	PCP-20T, HDM-135, HDM-136P, HB-121, HB-19□, HBM-100, HBM-310, HBR-191, HBU-112
ORP	RCP-20T, HDM-137/138, HB-123D, HBM-102/312
Fluoride ion	FBM-300, FBM-100, FB-31


**ELECTRODES**

The following electrodes and sensor chips are available,

Type of electrode	Model	Applications	Sensor chip for replacement
PH	ELCP-11-□F	General purpose (using standard glass membrane)	5081L
	ELCP-21-□F	Liquid containing fluoride (using hydrofluoric acid resistant glass membrane)	5082L
	ELCP-31-□F	Measurement in cold weather conditions (using low impedance glass membrane)	5080L
	ELCP-41-□F	High alkali liquid (using alkali resistant glass membrane)	5083L
ORP	ELCP-61-□F	General purpose (using platinum electrode)	2156L
	ELCP-71-□F	Cyanide decomposition process (using platinum electrode)	2157L
Fluoride-ion	ELCP-81-□F	Waste water (using lanthanum fluoride membrane)	7208L

□ Electrode cable length (5:5m, 10:10m) to be selected

**pH•ORP SYSTEM CONFIGURATION**

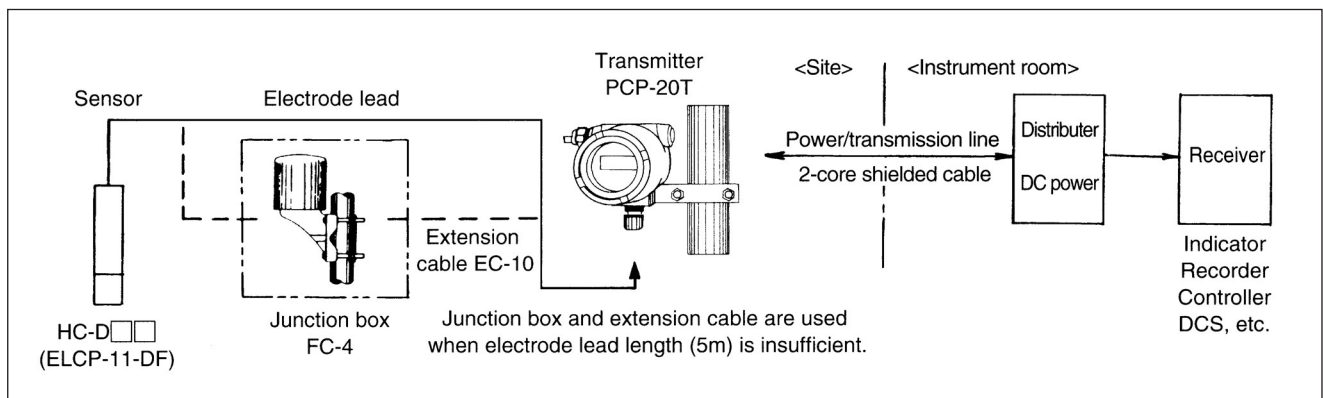

## pH ELECTRODE SPECIFICATION

The following four models are available, depending on the sensor chip to be used.

Model	ELCP-11-□F	ELCP-21-□F	ELCP-31-□F	ELCP-41-□F
Sensor chip, Glass membrane	General purpose	Hydrofluoric acid resistant type	For cold climate	Alkali resistant type
Measuring range	0 ~ 14 pH			
Durable temperature range	-10 ~ 85°C			
Operational temperature range	-5 ~ 80°C	-5 ~ 50°C	-5 ~ 80°C	
Operational pressure range	-0.09 ~ 0.7 MPa			
Inner electrode	Ag-AgCl electrode			
Reference electrode, inner liquid	Gelled KCl solution (Non supply type)			
Wetted materials	Epoxy resin. Tetra-fluoro ethylene resin. Fluoro rubber			
Glass membrane	Resistance of glass membrane	150 ~ 250 MΩ	150 ~ 250 MΩ	150 ~ 100 MΩ
	Alkali error	7mV	10mV	12mV
	Acid error	Less than 1mV		
	Linearity	Within ±1mV		
	Hydrofluoric acid resistant	1 Hour	6 Hours	0.5 Hour

Note 1) "Alkali error" is defined as the deviation from the theoretical value at pH12.8 (0.1 M NaOH), and "Acid error" is defined as the deviation from the theoretical value at pH1.1 (0.1 M HCl). "Linearity" is defined as the deviation from the value of pH6.86 after calibration at pH4.01 and pH9.18. "Hydrofluoric acid resistant" is described by the time at which glass membrane dissolves in 5% HF aqueous solution, and indicates the index of glass solubility against hydrofluoric acid.

Note 2) Hydrofluoric acid resistant glass is applicable for the sample containing hydrofluoric acid less than 1000 mg/L. The glass solubility against the sample containing fluoride ions may depend on pH value of sample. The sample with pH value less than 4pH where fluorides exist as fluoridic acid may dissolve glass electrode, but the sample with pH value over 4pH where fluorides exist as fluoride ions will not easily dissolve glass membrane even if the sample contains much fluorides.

## ORP ELECTRODE, SPECIFICATIONS


Model	ELCP-61-□F	ELCP-71-□F
Sensor Chip	Platinum	Alloy
Sensing membrane		
Measuring range	-2000 ~ 0 ~ 2000 mV	
Durable temperature range	-10 ~ 85°C	
Operational temperature range	-5 ~ 80°C	
Operational pressure range	-0.09 ~ 0.7 MPa	
Inner electrode	Ag-AgCl electrode	
Reference electrode, Inner liquid	Gelled KCl solution (Non-supply type)	
Wetted materials	Epoxy resin, Tetra-fluoro ethylene resin, Fluoro rubber	

## FLUORIDE ION ELECTRODE, SPECIFICATIONS

Model	ELCP-81-□F	
Sensor Chip	Lanthanum fluoride	
Sensing membrane	Single crystal	
Measuring range	0.1 ~ 10,000 mg/L F <sup>-</sup>	
Durable temperature range	-10 ~ 50°C	
Operational temperature range	-5 ~ 40°C	
Operational pressure range	-0.09 ~ 0.2 MPa	
Inner electrode	Ag-AgCl electrode	
Reference electrode, Inner liquid	Gelled KCl solution (Non-supply type)	
Wetted materials	Epoxy resin, Tetra-fluoro ethylene resin, Fluoro rubber	
Operational conditions	pH	5 ~ 9 pH
	Conductivity	Min. 500μ S/cm
	Flow rate	1 ~ 20 cm/s

**ELECTRODE**


The electrode is mounted on a holder with a pipe thread Rc<sup>3/4</sup>".

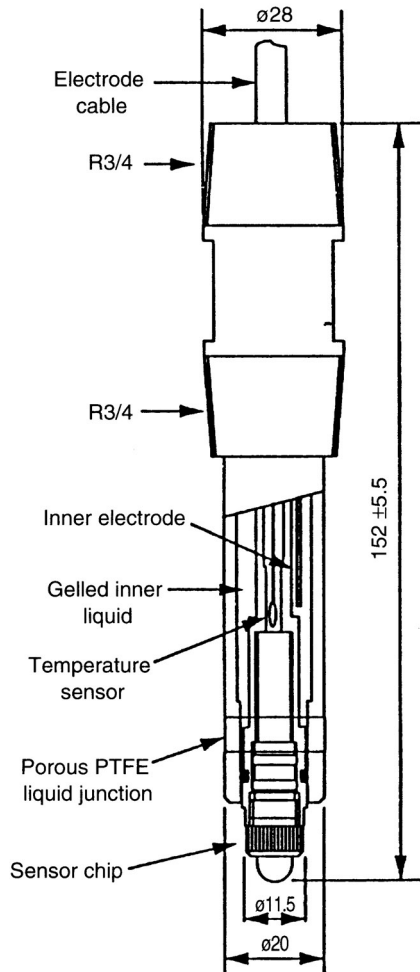


**SENSOR CHIP**

The sensor chip is attached to the electrode body by a rubber screw, of which, the sealing has a pressure resistance of more than 1 MPa.


**pH sensor chip**

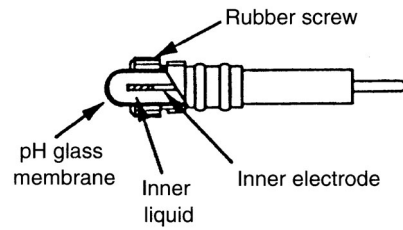

**ORP sensor chip**

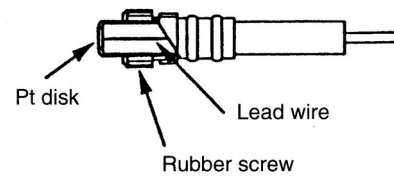


**F- ion sensor chip**

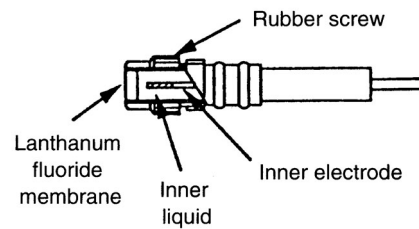


**FLOW-THROUGH TYPE HOLDER**


Model	Process connection	Wetted materials	Pressure range	Temperature range
HC-D86	Pipe thread Rc1/2 with plastic chamber	PP (Polypropylene)	0 ~ 0.15 MPa	-5 ~ 60°C
HC-D82	Pipe thread Rc1/2 with metallic chamber	Stainless Steel	0 ~ 0.45 MPa	-5 ~ 80°C
HC-D88	Flange (25A JIS 10K FF) with plastic chamber	PP (Polypropylene)	0 ~ 0.15 MPa	-5 ~ 80°C

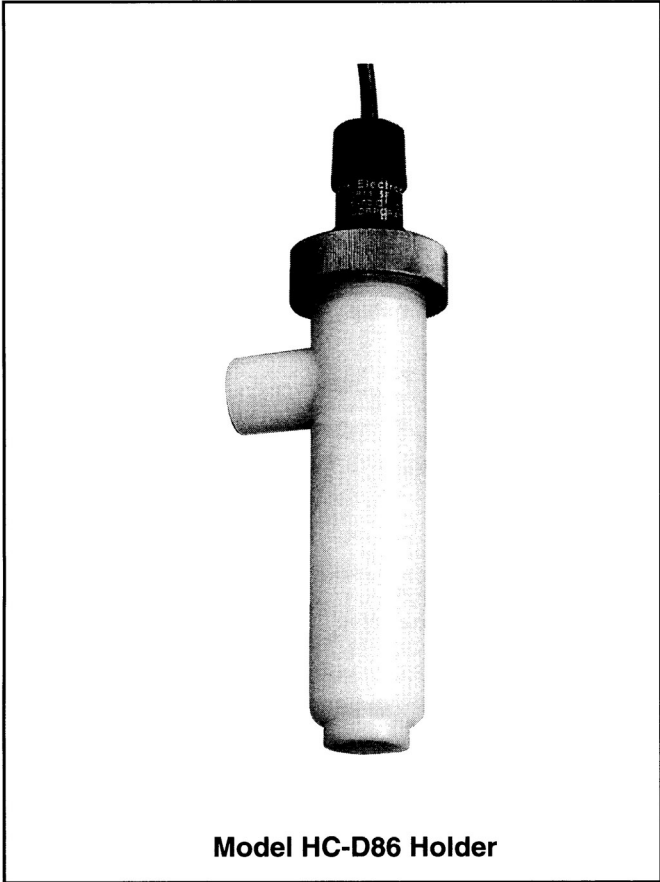


**Model HC-D86**

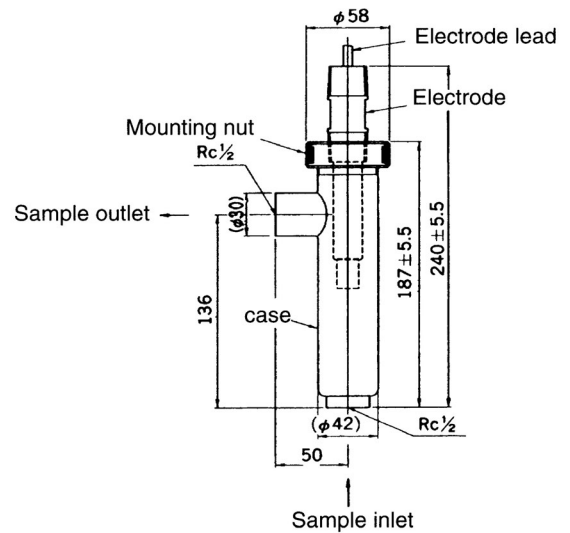

**Model HC-D82**

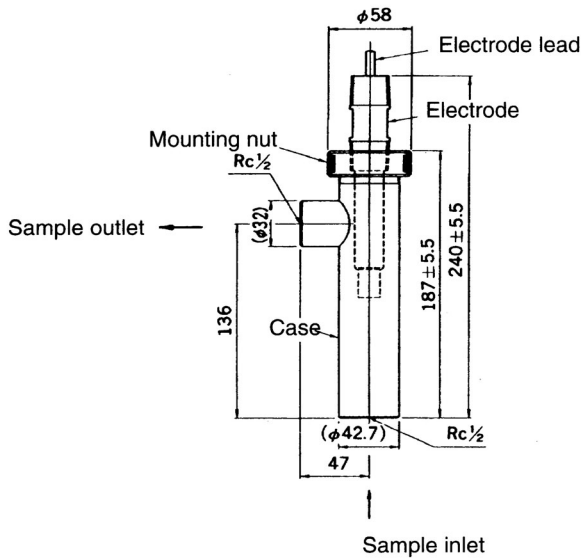



**Model HC-D88**

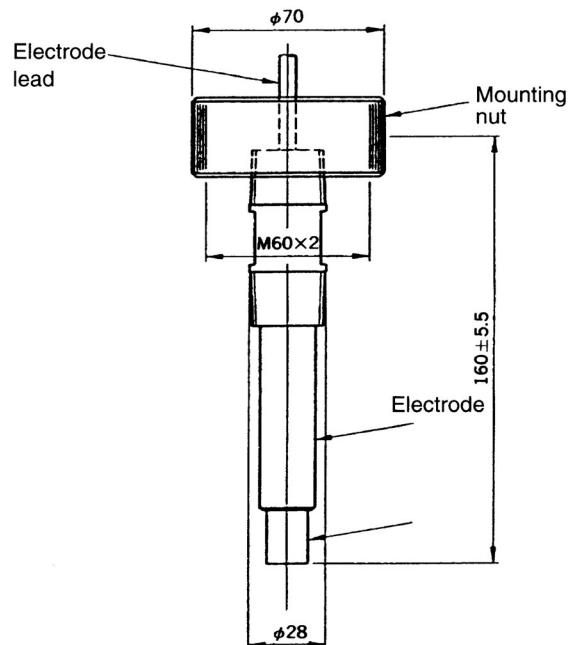

**IMMERSION TYPE HOLDER**

Model	Wetted materials	Temperature range	Applications
HC-D70C	PVC (Polyvinyl chloride)	-5 ~ 60°C	General purpose, Weather resistant
HC-D70F	PVDF (Polyvinylidene di-fluoride)	-5 ~ 80°C	High temperature resistant, Chemical resistant
HC-D70T	PFA (Perfluoro alkoxi ethylene)	-5 ~ 80°C	Chemical resistant
HC-D72	Stainless Steel	-5 ~ 95°C	High temperature resistant, Mechanical resistant
HC-D76	PP (Polypropylene)	-5 ~ 80°C	General purpose




Holder length: 0.5, 1, 1.5, 2m

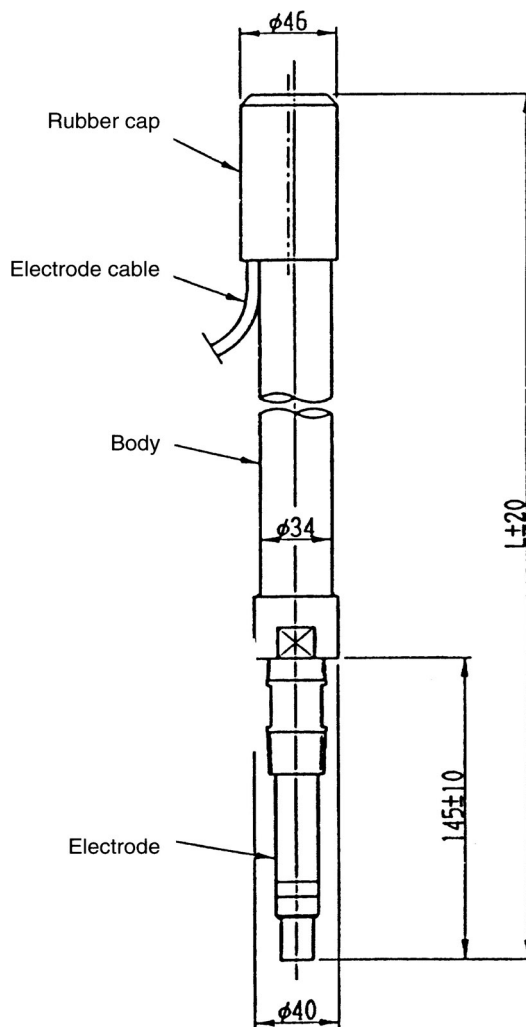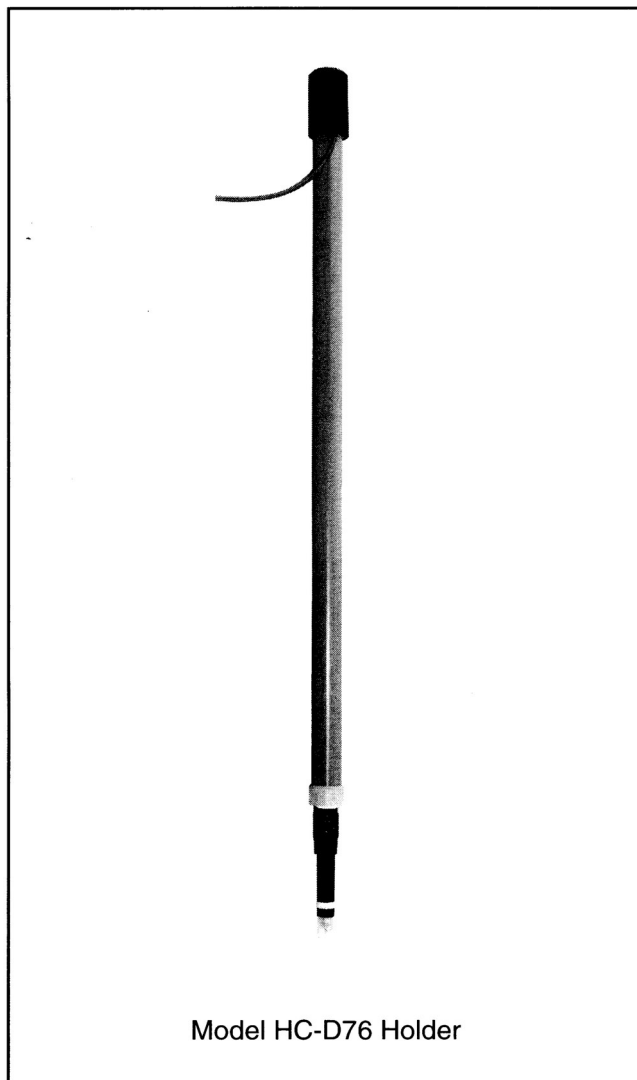

**DIP-IN TYPE HOLDER**

Model	Process connection	Wetted material	Temperature range
HC-D90	Dip in with plastic guide pipe	Polyvinyl chloride	-5 ~ 60°C
HC-D95	Dip in with metallic guide pipe	Stainless Steel	-5 ~ 80°C

Length of guide pipe: 0.5, 1, 1.5, 2, 2.5, 3, 3.5, 4, 4.5, 5 m

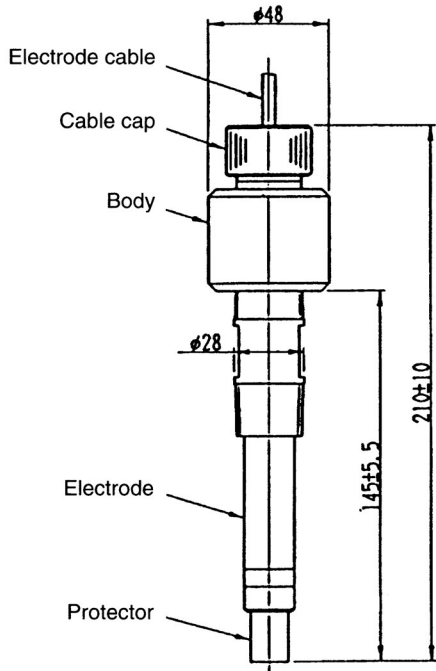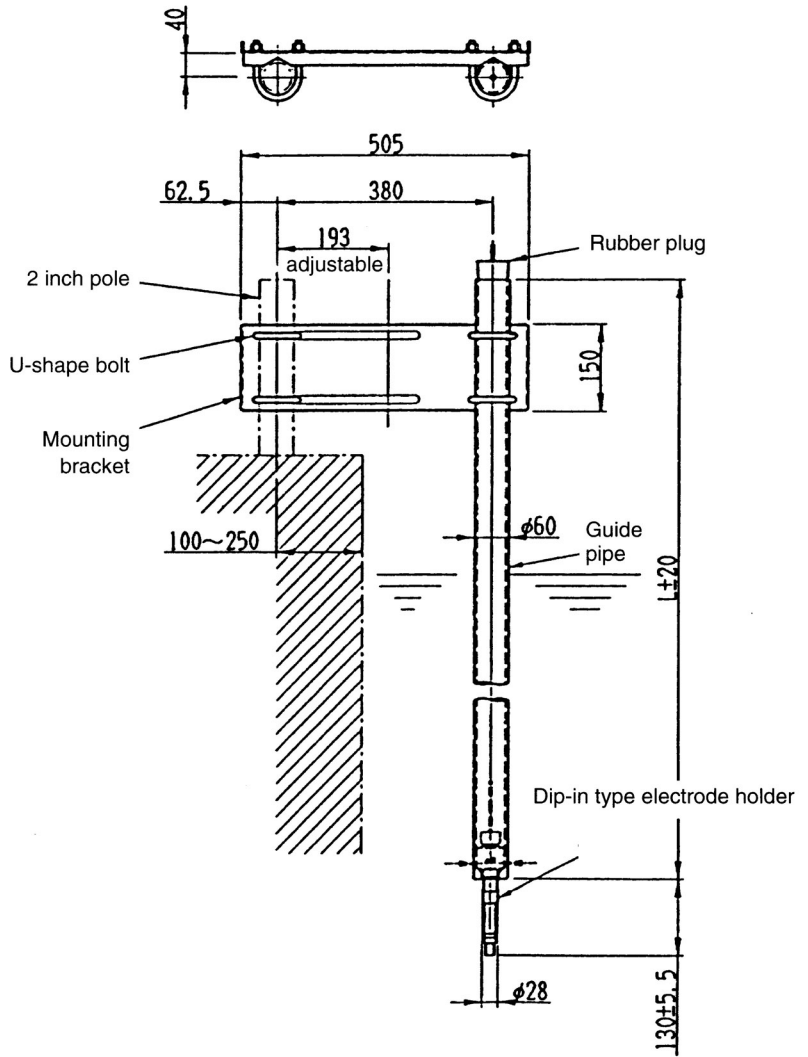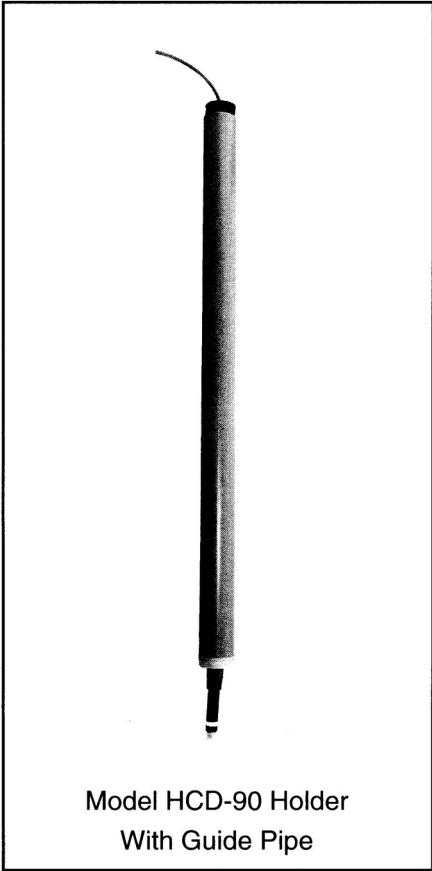



## pH STANDARD

DKK-TOA offer various pH standard solutions (500mL) and powder reagents (for 500mL solution).

DKK-TOA's Class 2 pH standard solutions are traceable to Japanese national standards and include the relevant certification.

### Class 2 pH Standard Solution

Description	pH value at 25°C and criteria	Bottle	Parts number
Phthalate pH standard solution, Class 2	4.01 ±0.015	500mL	143F501
Phosphate pH standard equimolal solution, Class 2	6.86 ±0.015	500mL	143F502
Tetraborate pH standard solution, Class 2	9.18 ±0.015	500mL	143F503

### pH Standard Solution

Description	pH value at 25°C	Accuracy	Bottle	Parts number
Oxalate pH standard solution	1.68	±0.02	500mL	143F063
0.01M oxalate pH standard solution	2.15	±0.02	500mL	143F091
Phthalate pH standard solution	4.01	±0.02	500mL	143F055
Phosphate pH standard equimolal solution	6.86	±0.02	500mL	143F056
Tetraborate pH standard solution	9.18	±0.02	500mL	143F057
Carbonate pH standard solution	10.01	±0.02	500mL	143F064

### Powder Reagent for pH Standard Solution

Description	pH value at 25°C	Quantity	Parts number
Powder reagent for oxalate pH standard solution	1.68	5 bags, each for 500mL solution	143F065
Powder reagent for 0.01M oxalate pH standard solution	2.15	5 bags, each for 500mL solution	143F090
Powder reagent for phthalate pH standard solution	4.01	5 bags, each for 500mL solution	143F060
Powder reagent for phosphate standard equimolal solution	6.86	5 bags, each for 500mL solution	143F061
Powder reagent for tetraborate pH standard solution	9.18	5 bags, each for 500mL solution	143F062
Powder reagent for carbonate pH standard solution	10.01	5 bags, each for 500mL solution	143F066

## ORP STANDARD

The ORP standard solution should be prepared by saturating phthalate pH standard solution with Quinhydrone when used.

Description	Quantity	Parts number
ORP standard solution (pH4.01 solution + Quinhydrone)	For 500mL solution	143F058
Powder reagent for ORP standard solution (pH4.01 powder and Quinhydrone)	5 bags, each for 500mL solution	143F089
Powder Quinhydrone for ORP standard solution (Quinhydrone, only)	5 bags, each for 500mL solution	143F059

## FLUORIDE ION STANDARD pH IONIC STRENGTH ADJUSTMENT BUFFER SOLUTION

Calibration standard liquid should be prepared to contain pH5-AB with a concentration of 1% to adjust pH value at 5 and to keep constant ionic strength. When sample contains interference components such as  $\text{Ca}^{2+}$ ,  $\text{Fe}^{3+}$  or  $\text{Al}^{3+}$  which will form chelate ions giving low readings, the addition of F-DIMAB to sample with 5~10% concentration will be effective to decompose the chelate ions.

Description	Concentration	Bottle	Part number
Fluoride ion standard liquid	1,000 mg/L $\text{F}^-$	500mL	143F077
PH5-AB	-	500mL	143A053
F-DIMAB	-	500mL	143F123

## CF51 CLEANER FOR pH ELECTRODES

CF51 cleaning liquid is used for cleaning of glass electrode. The aqueous solution with 5% hydrochloric acid and 1% hydrofluoric acid cleans the glass membrane of the electrode surface free of adhered fouling, by slightly dissolving the glass surface. This is best suited for insoluble fouling such as silica ( $\text{SiO}_2$ ) and calcium compounds ( $\text{CaF}_2$ ,  $\text{CaSO}_4$ ) which may increase the response time of electrode.

Description	Bottle	Part number
CF51 Cleaner	500mL	143C501

## DKK-TOA CORPORATION



## CAUTION

Do not operate products before consulting instruction manual.

### International Operations:

DKK-TOA Corporation  
29-10, 1-Chome, Takadanobaba, Shinjuku-ku, Tokyo 169-8648 Japan  
Tel: +81-3-3202-0225 Fax: +81-3-3202-5685

### Representative Office (Europe):

DKK-TOA European Representative  
St. Johns Innovation Centre, Cowley Rd., Cambridge CB4 0WS UK.  
Tel: +44 (0)1223-526471 Fax: +44 (0)1223-709239

<http://www.toadkk.co.jp>

Information and specifications are for a typical system and are subject to change without notice.